

Organ Dolly

Web lock and tightener threading instructions

Threading Instructions

Follow closely unit familiar with threading procedure.

Figure 1

Hold locking device in extreme outward position.

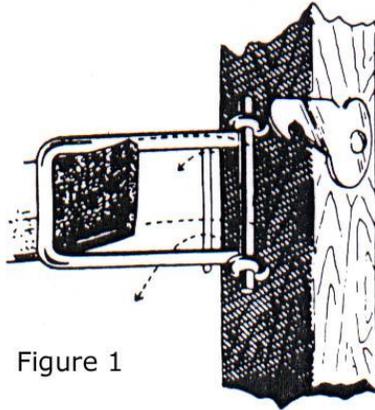


Figure 1

Figure 2

Strap is threaded through large opening around hinge post. Pull end through until in approximate adjustment.

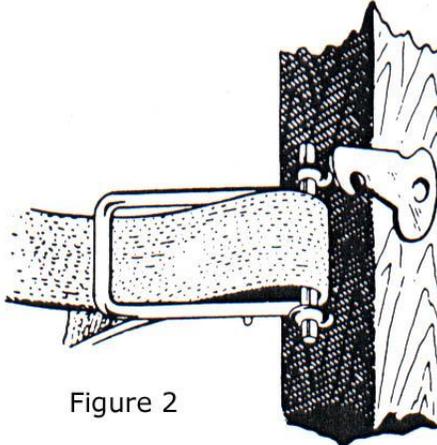


Figure 2

Figure 3

Swing locking device to locking position. Note: End of strap is inside of tightened strap if correctly threaded

Caution

Do not raise load until straps are tightened!

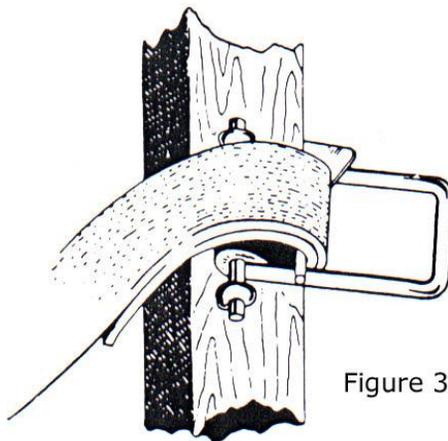


Figure 3